

DTK-adhesive


- Hygienic thanks to being autoclavable
- Proper bonding thanks to FGP insulating agent
- Suitable for direct and indirect use
- Bonding of all prosthetic materials:
 - On ceramic (e.max®) → Use K-Primer
 - On zirconia/ NPM / titanium → Use MKZ Primer
 - On precious metal alloys → Use MKZ Primer + MKZ EM-Aktivator
 - On BioHPP/ PEEK → Use visio.link




Adhesive protocol




Insulate screw channel, gingival area and shoulder of adhesive abutment and leave to dry.

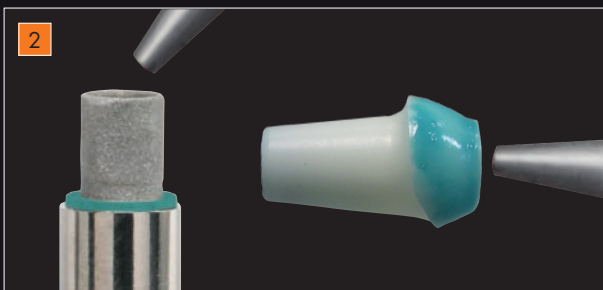

Sandblast with 110µm aluminium oxide: Pressure of 3 bar for titanium/NPM
2 bar for zirconia

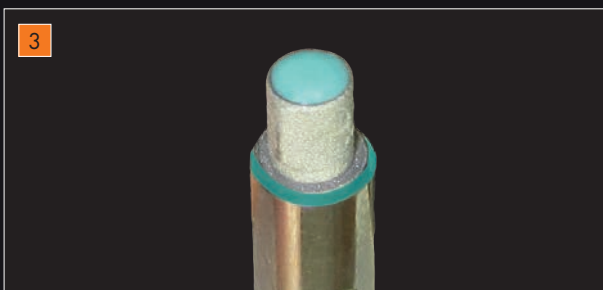


Seal screw channel with wax

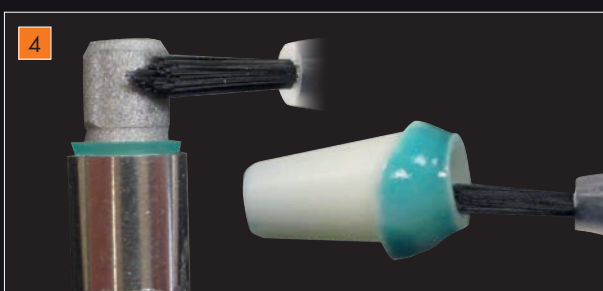

Apply MKZ Primer to titanium/NPM adhesive base and zirconia abutment.




Apply K-Primer on e-max® and MKZ Primer On titanium base.

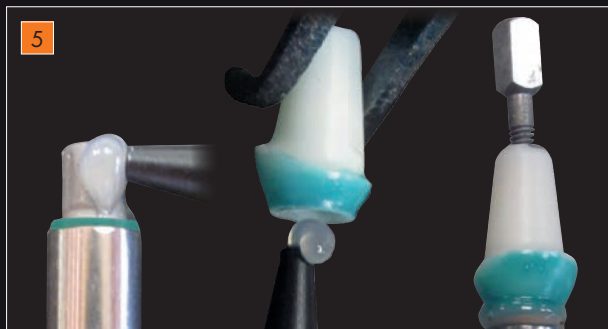


Apply DTK-adhesive (transparent or opaque), press abutment onto the adhesive base and then insert screw into the channel.




Polymerise with bre.Lux Power Unit2, for example.

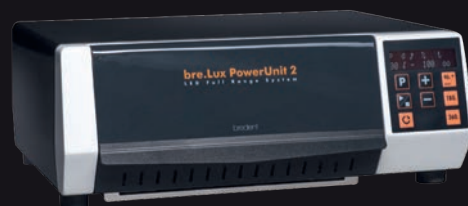

Remove the screw from the channel

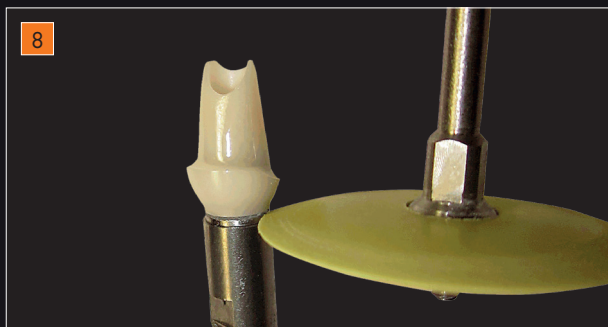

Sandblast abutment and remove excess

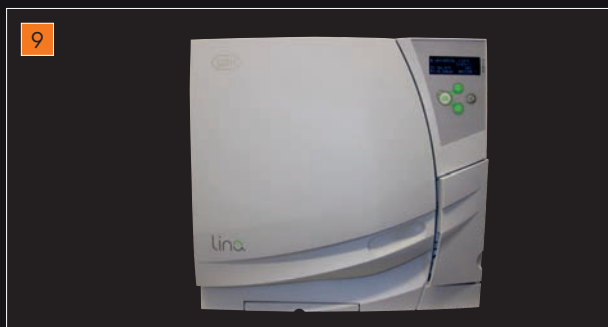

Bonded abutments can be sterilised.

Note! When using translucent and high-translucent zirconia abutments, contact manufacturer for information about hydrothermal stability achieved by aluminium oxide doping!

bredent
group

009894GB-20180329

Mistake and subject to change reserved



All names marked with ® or ™ are protected brands and/or company names or third-party rights holders.